

**GRAVITY PROBE B
PROCEDURE FOR
GSE CERTIFICATION**

DISCONNECT TM&A FROM SMD

P0790 Rev. -

10 January 2001

Prepared by: *B. Clarke*

Approvals:

Program Responsibility	Signature	Date
B. Clarke Test Engineer		
D. Murray Cryogenic Engineer		
M. Taber Payload Test Director		
R. Whelan GP-B System Engineering		
D. Ross GP-B Quality Assurance		
B. Muhlfelder GP-B Payload Technical Manager		

NOTES:

Level of QA required during performance of this procedure:

Stanford QA Representative

Government QA Representative

All redlines must be approved by QA

Revision Record:

Rev	Rev Date	ECO #	Summary Description

Acronyms and Abbreviations:

Acronym / Abbreviation	Meaning
TM&A	Temperature Monitor and Alarm
SMD	Science Mission Dewar

Table of Contents

A Scope	4
B Requirements Verification	4
C Configuration Requirements.....	4
D Hardware Required	4
E Software Required	4
F Procedures Required.....	5
G Equipment Pretest Requirements	6
H Personnel Requirements.....	6
I Safety Requirements.....	6
J General Instructions.....	6
K References and Applicable Documents.....	6
L Operations.....	7

A Scope

This procedure is used to disconnect the Temperature Monitor and Alarm system (TM&A) from the Science Mission Dewar (SMD).

B Requirements Verification

B.1 Requirements Cross-Reference

None.

B.2 Expected Data for verification per requirement

None.

C Configuration Requirements

None.

D Hardware Required

D.1 Commercial test equipment

Manufacturer	Model	Serial Number	Calibr. Exp. Date

D.2 Mechanical/Electrical Special test equipment

Description	Part No.	Rev. no.	Serial No.	Certification Date

D.3 Tools

Description	No. Req'd

D.4 Expendables

Description	Quantity

E Software Required

E.1 Flight Software

Flight Software Name	Version No.
MSS (Mission Support Software)	
SUS (Start Up Software)	
BSS (Boot Strap Software)	
OSS (Operating System Software)	
SSW (SQUID/ST Support Software)	
GSW (GSS Support Software)	

E.2 CSTOL Scripts

CSTOL Script Name	Version No.

E.3 SPC Scripts

SPC Script Name	Version No.

E.4 Test Support Software

Test Software Name	Version No.

F Procedures Required

Procedure Name	Procedure No.

G Equipment Pretest Requirements

Equipment	Serial No.	Test Required	Proc. No.	Test Performed	
				Date	By

H Personnel Requirements

Test Leader

The Test Leader shall be Mike Taber, Dave Murray or Bruce Clarke. He has overall responsibility for the implementation of this procedure.

Other Personnel

All personnel participating in this procedure shall work under the direction of the Test Leader who shall determine whether the person is qualified. Different people will likely be designated at different times. For this procedure, participating engineers are expected to be (at various times) Mike Taber, Dave Murray, Tom Welsh, Jim Maddocks and Bruce Clarke.

The QA program office shall be notified 24 hours prior to the start of this procedure. A Quality Assurance Representative designated by D. Ross shall review any discrepancy noted during this procedure, and approve its disposition.

I Safety Requirements

Extreme care must be taken to avoid accidentally bumping the Probe or damaging the connectors. Connectors should be inspected for bent pins and/or debris prior to mating. Connector savers or equivalent adapters shall be used to protect the connector pins from damage during the measurements. A properly grounded ESD wrist strap must be worn while mating to or de-mating from Probe connectors. **All mate/demates involving flight connectors shall be logged.**

J General Instructions


- J.1 Redlines can be initiated by the Test Leader or their designate and must be approved by QA.
- J.2 Any nonconformance or test anomaly should be reported by a Discrepancy Report. Refer to the Quality Plan, P0108, for guidance. Do not alter or break test configuration if a test failure occurs; notify quality assurance.
- J.3 Only the Test Leader has the authority to exit/terminate this test or to perform a retest.

K References and Applicable Documents

L Operations

TM&A Configuration

The figure below shows the set-up of the TM&A as it is intended to be used on the SMD/PAYLOAD. The cable connections to the SMD/PAYLOAD are K/A-D-G (K = 63-pin female, A, D and G = 66-pin female) and two 5-conductor ENDEVCO cables (male/female, 9-pin D-style connector).

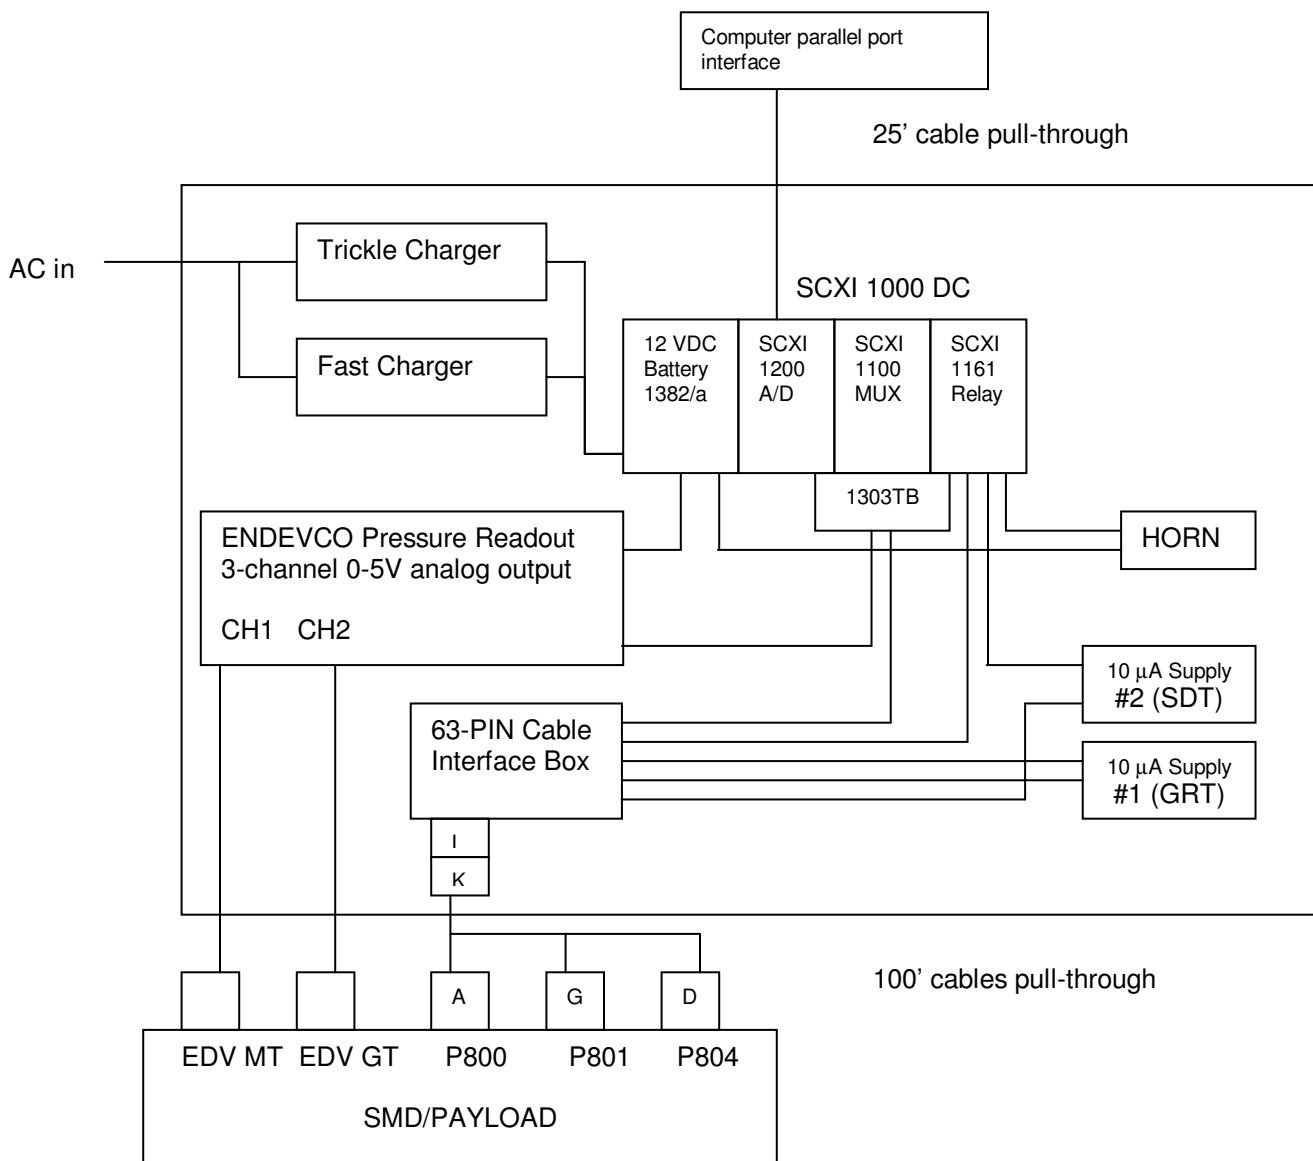

L.1 Check that all the TM&A components are powered down and that the horn is switched off.

AC in	unplugged
SCXI DC 1000	OFF
ENDEVCO	OFF
10 μ A #1 (GRT)	OFF
10 μ A #1 (SDT)	OFF
Laptop Computer	OFF
Horn defeat	ON

L.2 Disconnect the TM&A cables from the SMD and from the ENDEVCO heads. Disconnect the laptop computer interface to the SCXI chassis.

L.2.1 Disconnect cable K/A-D-G from the interface box (connector K to L) and from the SMD (A from P800, G from P801, D from P804) and stow.

L.2.2 Disconnect the main tank and guard tank ENDEVCO cables from the ENDEVCO readout and from the ENDEVCO heads and stow.

L.2.3 Disconnect the parallel interface cable from the parallel port of the laptop computer and from the SCXI 1200 and stow.

Task completed.

Completed by: _____
Witnessed by: _____
Date: _____
Time: _____

TM&A CABLING

		A	K	L		1303	1161	other
Device	function	P800/P1			L jumpers			
T22D top lead bag /a	-	-	1	1		GND		
	V+	6	2	2		CH0+		
	V-	12	3	3		CH0-		
	-	-	4	4	10	GND		
GRT	I+	1	5	5			NO(0)	
	I-	5	6	6	11			
T23D top lead bag /b	shield	-	7	7		GND		
	V+	28	8	8		CH1+		
	V-	29	9	9		CH1-		
	shield	-	10	10	34			
GRT	I+	19	11	11	6			
	I-	20	12	12	35			
T09D main tank bottom	shield	-	13	13		GND		
	V+	16	14	14		CH2+		
	V-	23	15	15		CH2-		
	shield	-	16	16		GND		
SDT	I+	9	17	17			NO(1)	
	I-	15	18	18				10uA(-) SDT
T15D guard tank /a	shield	-	19	19		GND		
	V+	7	20	20		CH3+		
	V-	8	21	21		CH3-		
SDT	shield	-	22	22		GND		
	I+	2	23	23			NO(2)	
	I-	3	24	24				10uA(-) SDT
T24D fill valve V13	shield	-	25	25		GND		
	V+	11	26	26		CH4+		
	V-	18	27	27		CH4-		
	shield	-	28	28		GND		
	I+	4	29	29			NO(3)	
SDT	I-	10	30	30				10uA(-) SDT
Device	function	D	K	L		1303	1161	other
		P804/P5			L jumpers			
T20D top lead bag /c	-	-	31	31		GND		
	V+	35	32	32		CH5+		
	V-	36	33	33		CH5-		
	-	-	34	34	40			
GRT	I+	26	35	35	12			
	I-	27	36	36	41			
T21D top lead bag /d	shield	-	37	37		GND		
	V+	16	38	38		CH6+		
	V-	23	39	39		CH6-		
GRT	shield	-	40	40	46			
	I+	9	41	41	36			
	I-	15	42	42	47			
Device	function	D	K	L		1303	1161	other
		P801/P2			L jumpers			
T01D station 200 /a	-	-	43	43		GND		
	V+	16	44	44		CH7+		
	V-	23	45	45		CH7-		
GRT	-	-	46	46	52			
	I+	9	47	47	42			
	I-	15	48	48	53			
T10D MT top /a	shield	-	49	49		GND		
	V+	62	50	50		CH8+		
	V-	63	51	51		CH8-		

GRT	shield	-	52	52	46			
	I+	56	53	53	48			
	I-	57	54	54				10uA(-) GRT
T05D VCS-1 Bottom	shield	-	55	55		GND		
	V+	28	56	56		CH9+		
	V-	29	57	57		CH9-		
SDT	shield	-	58	58		GND		
	I+	19	59	59			NO(4)	
	I-	20	60	60				10uA(-) SDT
T08D HEX-4	shield	-	61	61		GND		
	V+	34	62	62		CH10+	NO(5)	
	V-	43	63	63		CH10-		10uA(-) SDT
SDT	shield	-						
	I+	17						
	I-	25						

ENDEVCO and Spare A/D CHANNELS

		1303			1303
spare 63-pin	ENDEVCO		spare 63-pin	ENDEVCO	
	CH1-pin	CH11+	24		GND
	CH1-shield	CH11-	25		CH22+
		GND	26		CH22-
	CH2-pin	CH12+	27		GND
	CH2-shield	CH12-	28		CH23+
		GND	29		CH23-
	CH3-pin	CH13+	30		GND
	CH3-shield	CH13-	31		CH24+
		GND	32		CH24-
1		CH14+	33		GND
2		CH14-	34		CH25+
3		GND	35		CH25-
4		CH15+	36		GND
5		CH15-	37		CH26+
6		GND	38		CH26-
7		CH16+	39		GND
8		CH16-	40		CH27+
9		GND	41		CH27-
10		CH17+	42		GND
11		CH17-	43		CH28+
12		GND	44		CH28-
13		CH18+	45		GND
14		CH18-	46		CH29+
15		GND	47		CH29-
16		CH19+	48		GND
17		CH19-	49		CH30+
18		GND	50		CH30-
19		CH20+	51		GND
20		CH20-	52		CH31+
21		GND	53		CH31-
22		CH21+	54		GND
23		CH21-			

CURRENT SOURCE AND BATTERY TO 1161 RELAY

1161		10 uA GRT	10uA SDT	12VDC
	1161 jumper			
NC(0)				
COM(0)		10 uA (+)		
NO(0)				
NC(1)				
COM(1)	COM(2)		10 uA (+)	
NO(1)				
NC(2)				
COM(2)	COM(3)			
NO(2)				
NC(3)				
COM(3)	COM(4)			
NO(3)				
NC(4)				
COM(4)	COM(5)			
NO(4)				
NC(5)				
COM(5)	COM(4)			
NO(5)				
NC(6)				
COM(6)				
NO(6)				
NC(7)				
COM(7)				12 V (+)
NO(7)				

ENDEVCO CABLES

pin #	function	color
4		white
5		green
7		red
8		black
9	shield	none

Sensor end = female 9-pin D-style
Readout end = male 9-pin D-style